


Gelator 26 (1* reaction)

UNIVERSITY OF
Southampton

AVIIIHD400 [3]

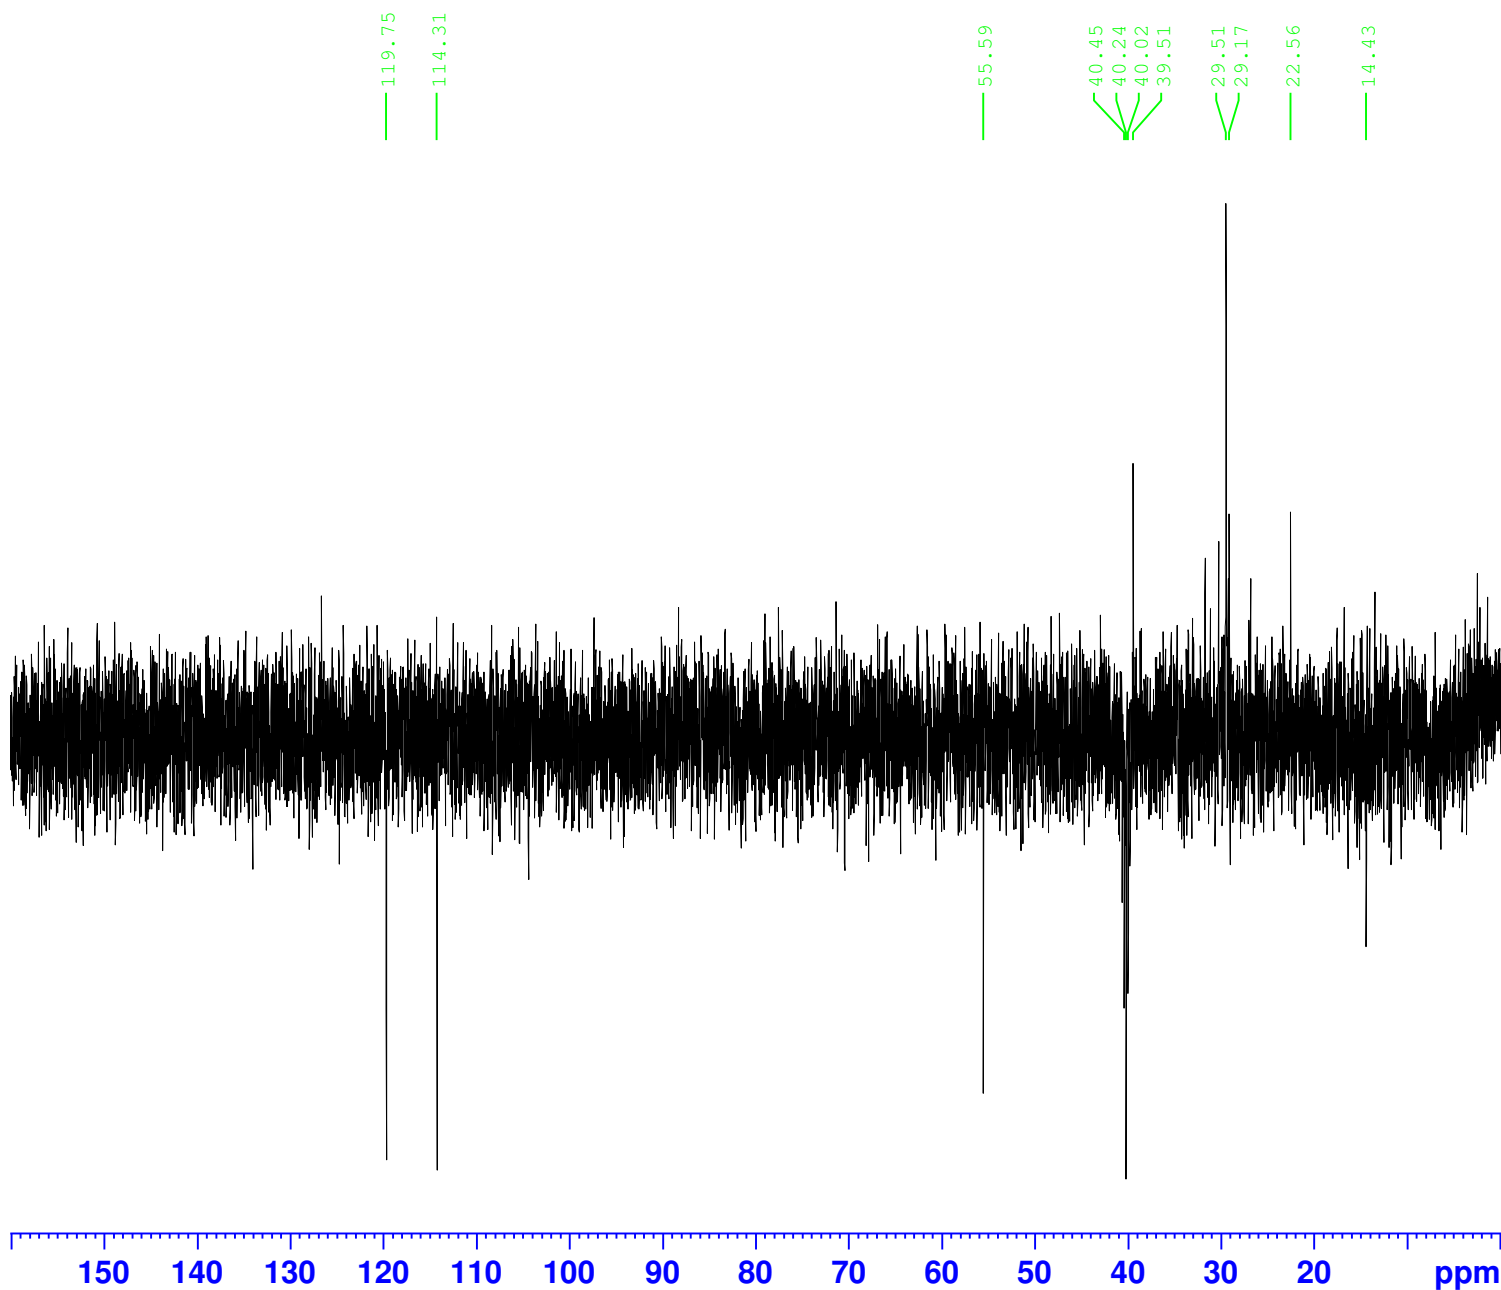

Current Data Parameters
NAME se0514fp1
EXPNO 12
PROCNO 1

F2 - Acquisition Parameters
Date_ 20140905
Time 17.30
INSTRUM spect
PROBHD 5 mm PABBO BB/
PULPROG deptsp135
TD 65536
SOLVENT DMSO
NS 256
DS 4
SWH 16129.032 Hz
FIDRES 0.246110 Hz
AQ 2.0316160 sec
RG 212.69
DW 31.000 usec
DE 6.50 usec
TE 298.0 K
CNST2 145.0000000
D1 2.00000000 sec
D2 0.00344828 sec
D12 0.00002000 sec
TD0 1

===== CHANNEL f1 =====
SFO1 100.6208171 MHz
NUC1 13C
P1 7.97 usec
P13 2000.00 usec
PLW0 0 W
PLW1 101.00000000 W
SPNAM[5] Crp60comp.4
SPOAL5 0.500
SPOFFS5 0 Hz
SPW5 9.80230045 W

===== CHANNEL f2 =====
SFO2 400.1312797 MHz
NUC2 1H
CPDPRG[2] waltz16
P3 7.00 usec
P4 14.00 usec
PCPD2 70.00 usec
PLW2 32.00000000 W
PLW12 0.31999999 W

F2 - Processing parameters
SI 32768
SF 100.6127690 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40