


AVIIIHD400 [3]

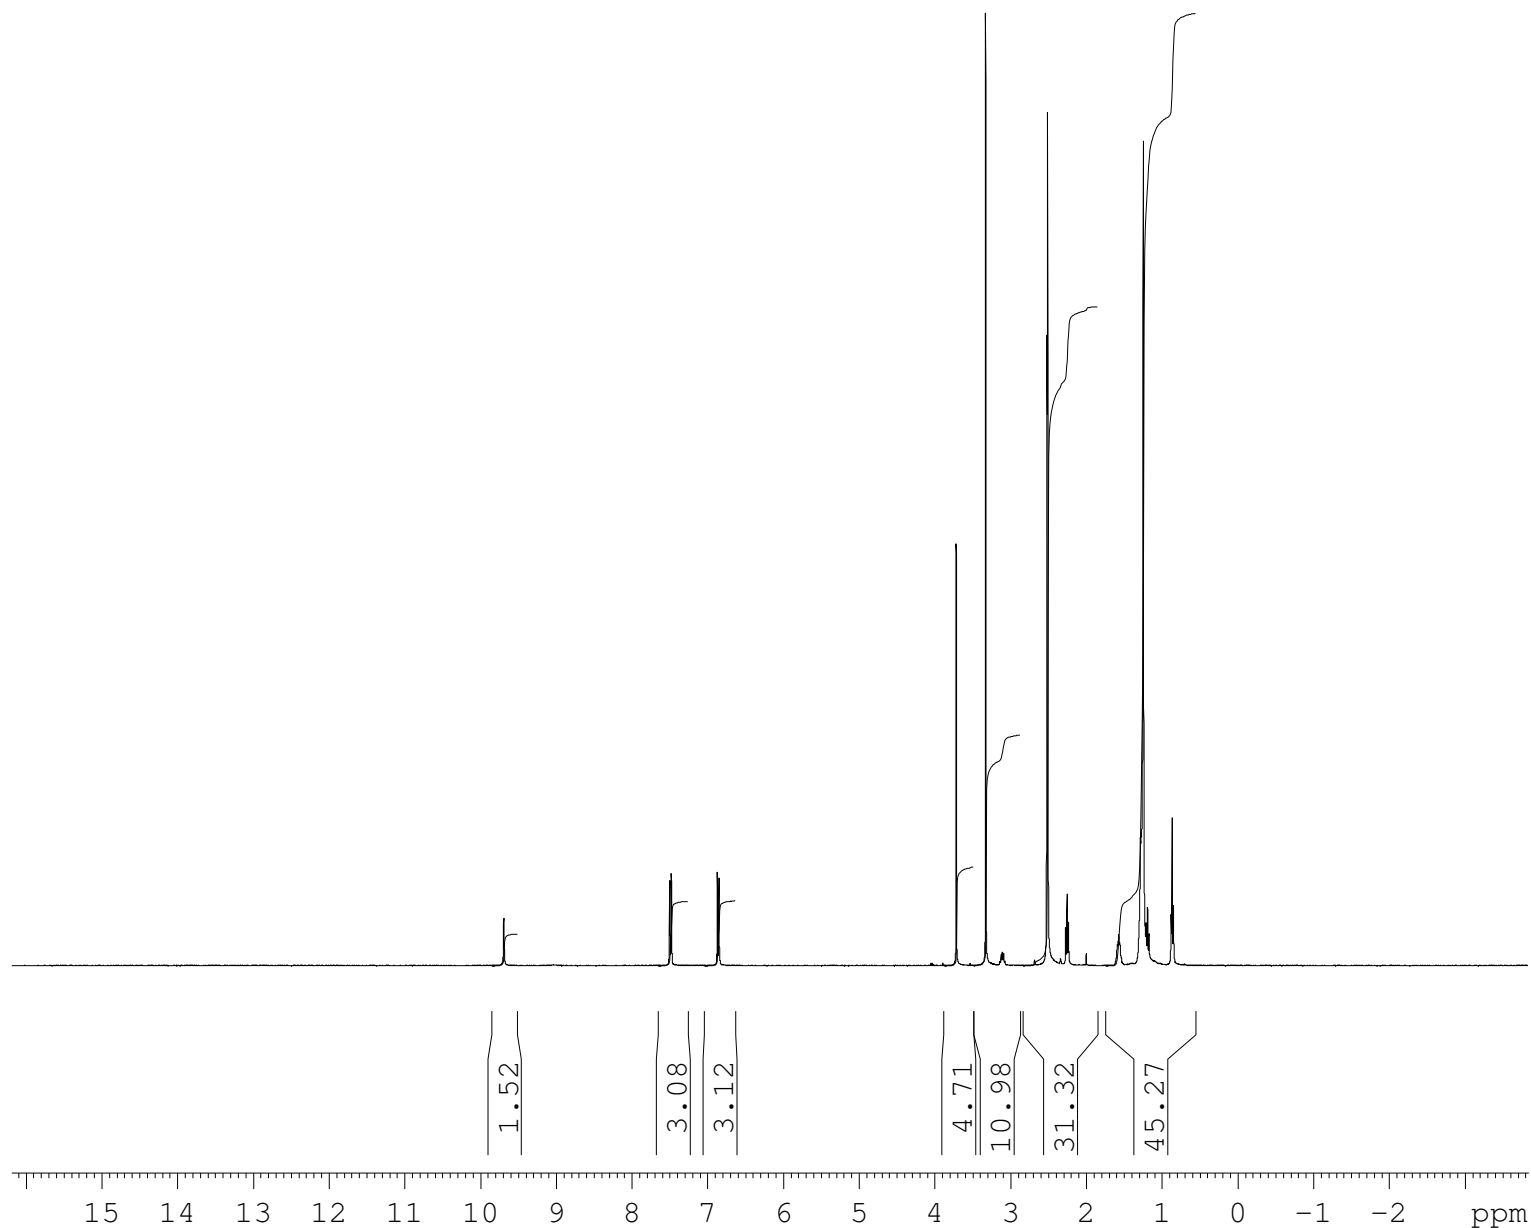

## Current Data Parameters

NAME nv2814fp1  
EXPNO 10  
PROCNO 1

## F2 - Acquisition Parameters

Date\_ 20141129  
Time 0.23  
INSTRUM spect  
PROBHD 5 mm PABBO BB/  
PULPROG zg30  
TD 65536  
SOLVENT DMSO  
NS 16  
DS 2  
SWH 8012.820 Hz  
FIDRES 0.122266 Hz  
AQ 4.0894465 sec  
RG 100.45  
DW 62.400 usec  
DE 6.50 usec  
TE 298.0 K  
D1 1.00000000 sec  
TD0 1

## ===== CHANNEL f1 =====

SFO1 400.1324710 MHz  
NUC1 1H  
P1 7.00 usec  
PLW1 32.00000000 W

## F2 - Processing parameters

SI 65536  
SF 400.1300000 MHz  
WDW EM  
SSB 0  
LR 0.30 Hz