


Gelator 11



AVIIIH400 [3]

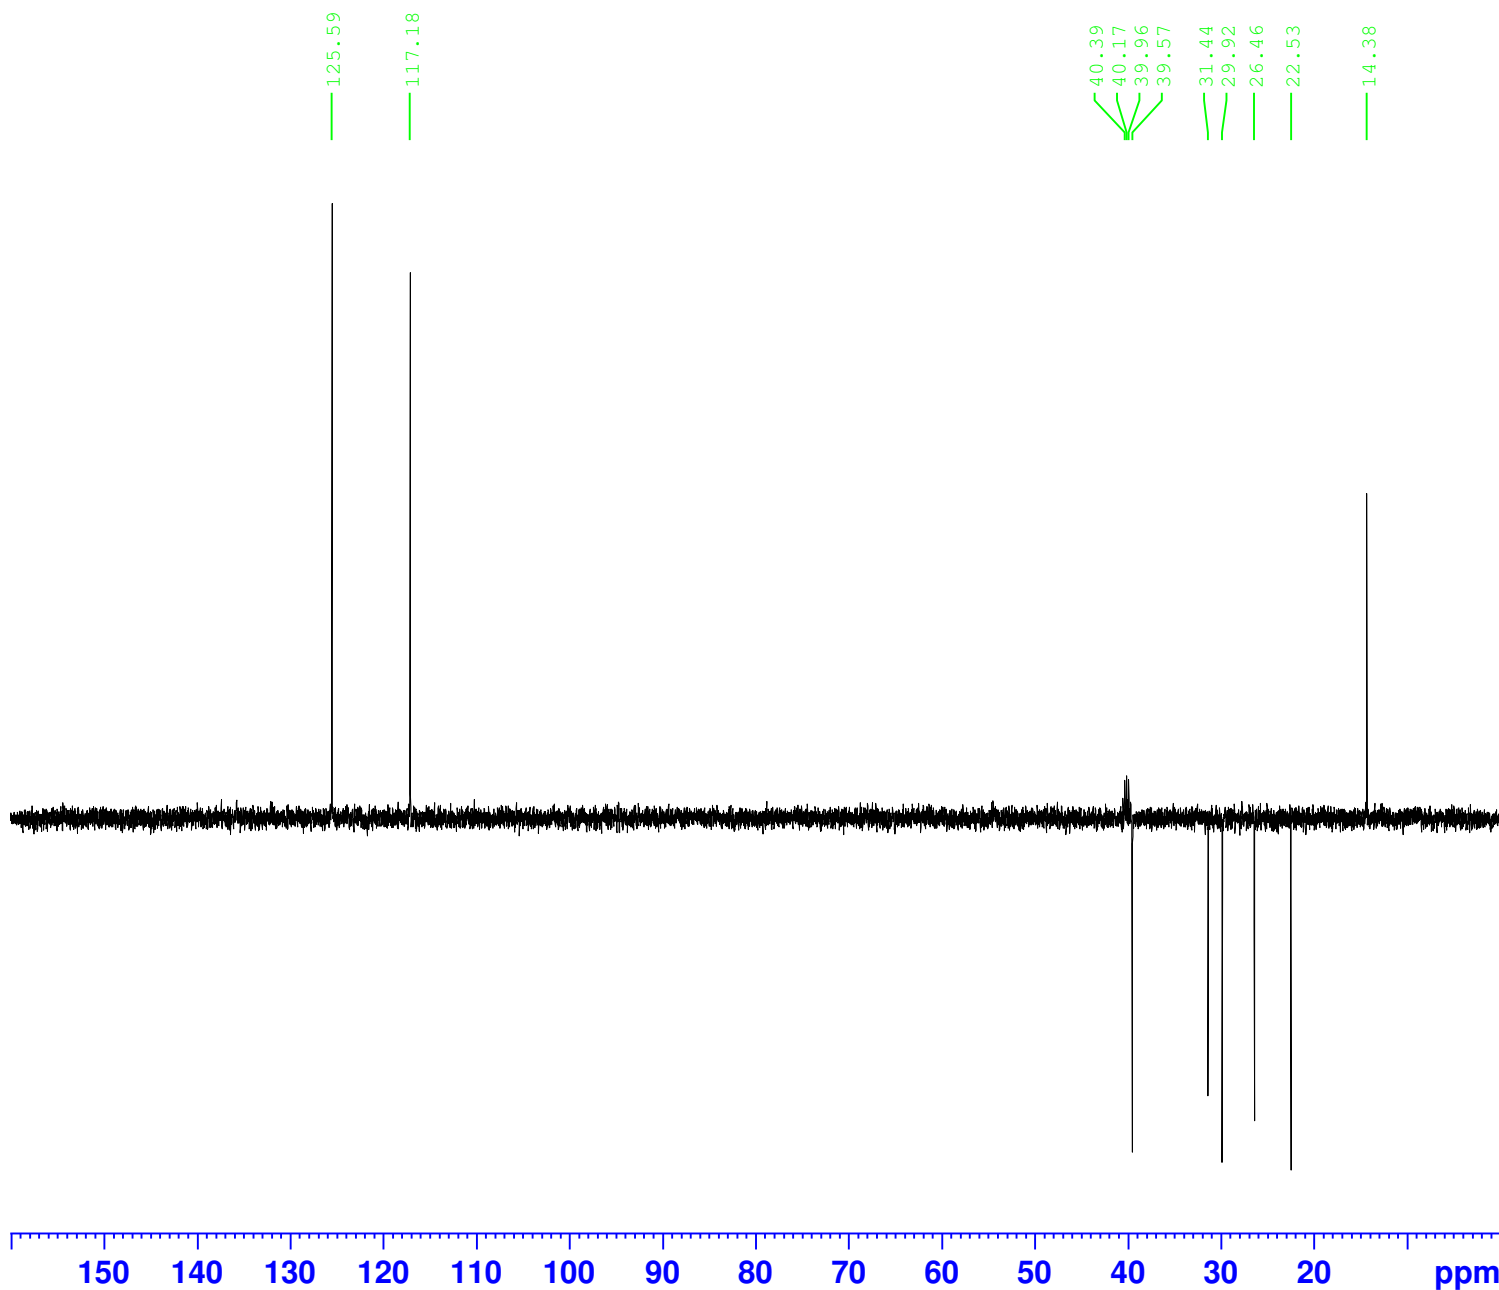

Current Data Parameters  
NAME ju0414fp2  
EXPNO 12  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20140604  
Time 12.36  
INSTRUM spect  
PROBHD 5 mm PABBO BB/  
PULPROG deptspl35  
TD 65536  
SOLVENT DMSO  
NS 256  
DS 4  
SWH 16129.032 Hz  
FIDRES 0.246110 Hz  
AQ 2.0316160 sec  
RG 212.69  
DW 31.000 usec  
DE 6.50 usec  
TE 298.0 K  
CNST2 145.0000000  
D1 2.00000000 sec  
D2 0.00344828 sec  
D12 0.00002000 sec  
TD0 1

===== CHANNEL f1 =====  
SFO1 100.6208171 MHz  
NUC1 13C  
P1 7.97 usec  
P13 2000.00 usec  
PLW0 0 W  
PLW1 101.00000000 W  
SPNAM[5] Crp60comp.4  
SPOAL5 0.500  
SPOFFS5 0 Hz  
SPW5 9.80230045 W

===== CHANNEL f2 =====  
SFO2 400.1312797 MHz  
NUC2 1H  
CPDPRG[2] waltz16  
P3 7.00 usec  
P4 14.00 usec  
PCPD2 70.00 usec  
PLW2 32.00000000 W  
PLW12 0.31999999 W

F2 - Processing parameters  
SI 32768  
SF 100.6127690 MHz  
WDW EM  
SSB 0  
LB 1.00 Hz  
GB 0  
PC 1.40