


Gelator 24 (1\* reaction) 2\*

UNIVERSITY OF  
Southampton

AVIIIHD400 [3]

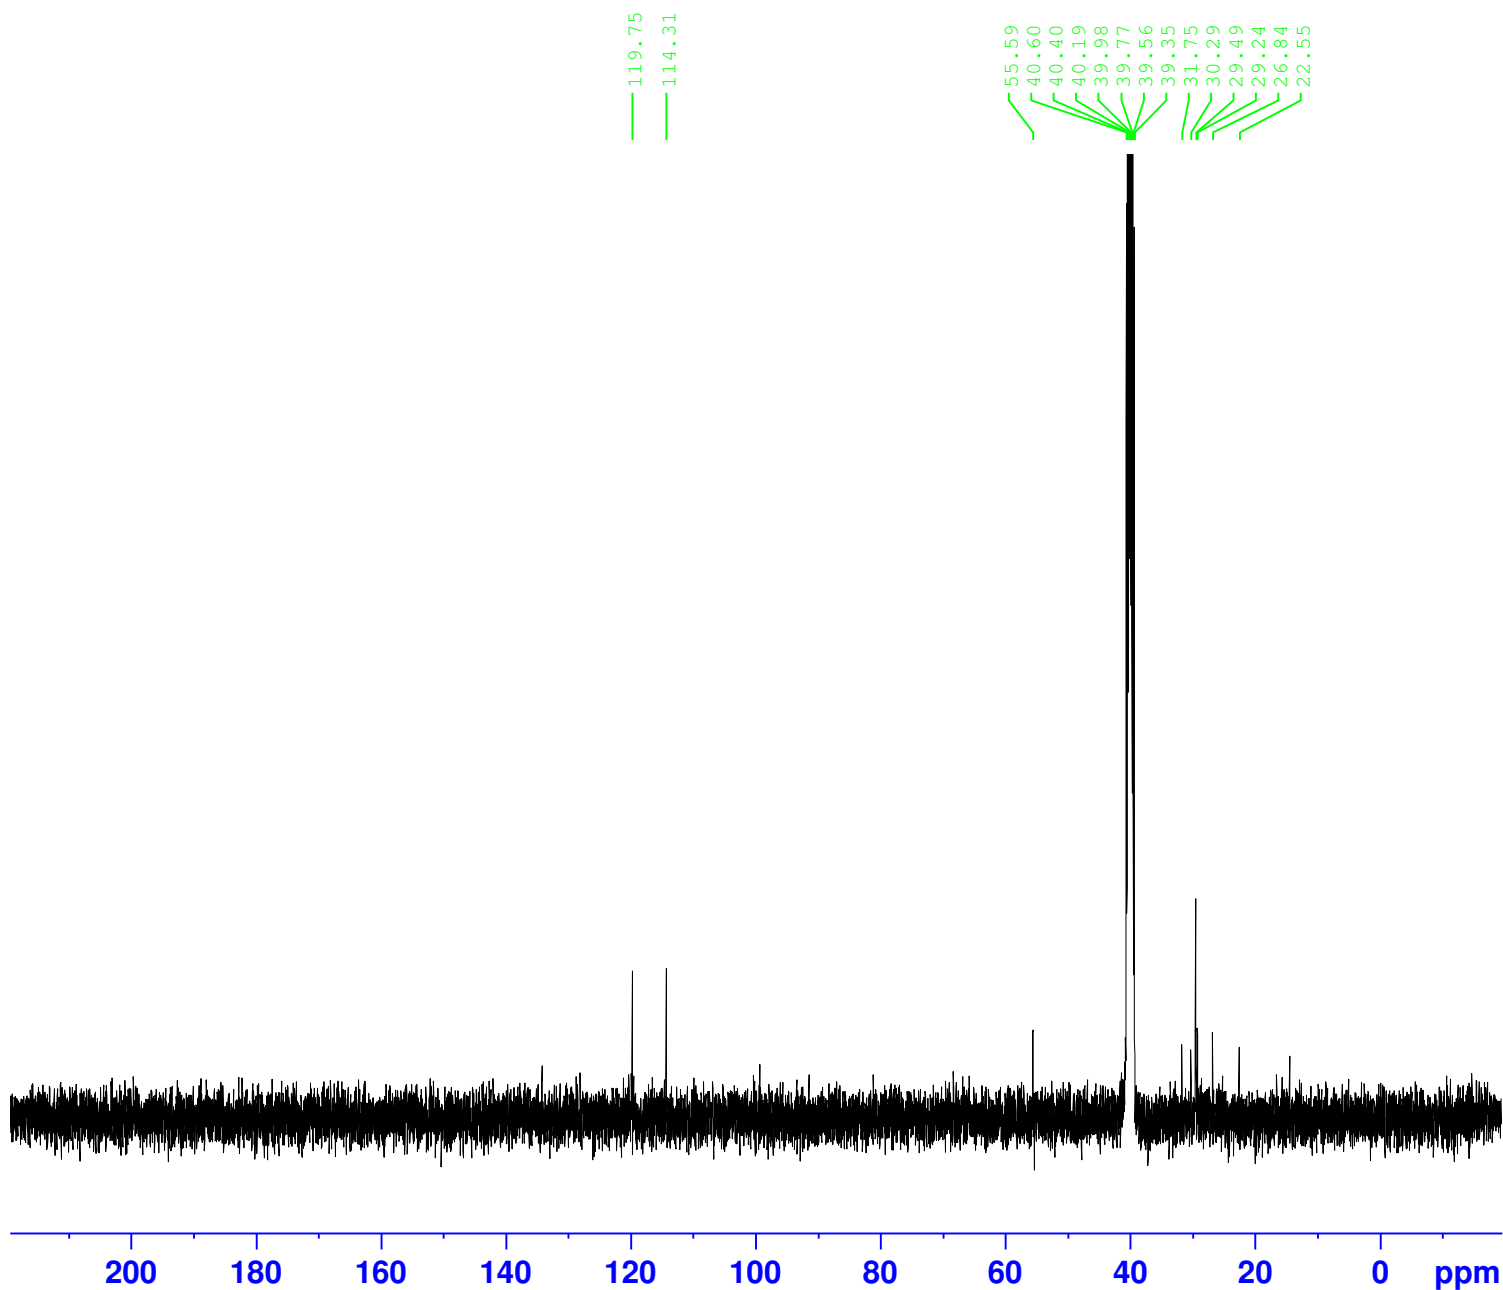

Current Data Parameters  
NAME se0514fp2  
EXPNO 11  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20140905  
Time 18.04  
INSTRUM spect  
PROBHD 5 mm PABBO BB/  
PULPROG zgpg30  
TD 65536  
SOLVENT DMSO  
NS 512  
DS 4  
SWH 24038.461 Hz  
FIDRES 0.366798 Hz  
AQ 1.3631488 sec  
RG 212.69  
DW 20.800 usec  
DE 6.50 usec  
TE 298.0 K  
D1 2.00000000 sec  
D11 0.03000000 sec  
TD0 1

===== CHANNEL f1 =====  
SFO1 100.6228293 MHz  
NUC1 13C  
P1 7.97 usec  
PLW1 101.00000000 W

===== CHANNEL f2 =====  
SFO2 400.1316005 MHz  
NUC2 1H  
CPDPRG[2] waltz16  
PCPD2 70.00 usec  
PLW2 32.00000000 W  
PLW12 0.31999999 W  
PLW13 0.15680000 W

F2 - Processing parameters  
SI 32768  
SF 100.6127690 MHz  
WDW EM  
SSB 0  
LB 1.00 Hz  
GB 0  
PC 1.40