


AVIIIHD400 [3]

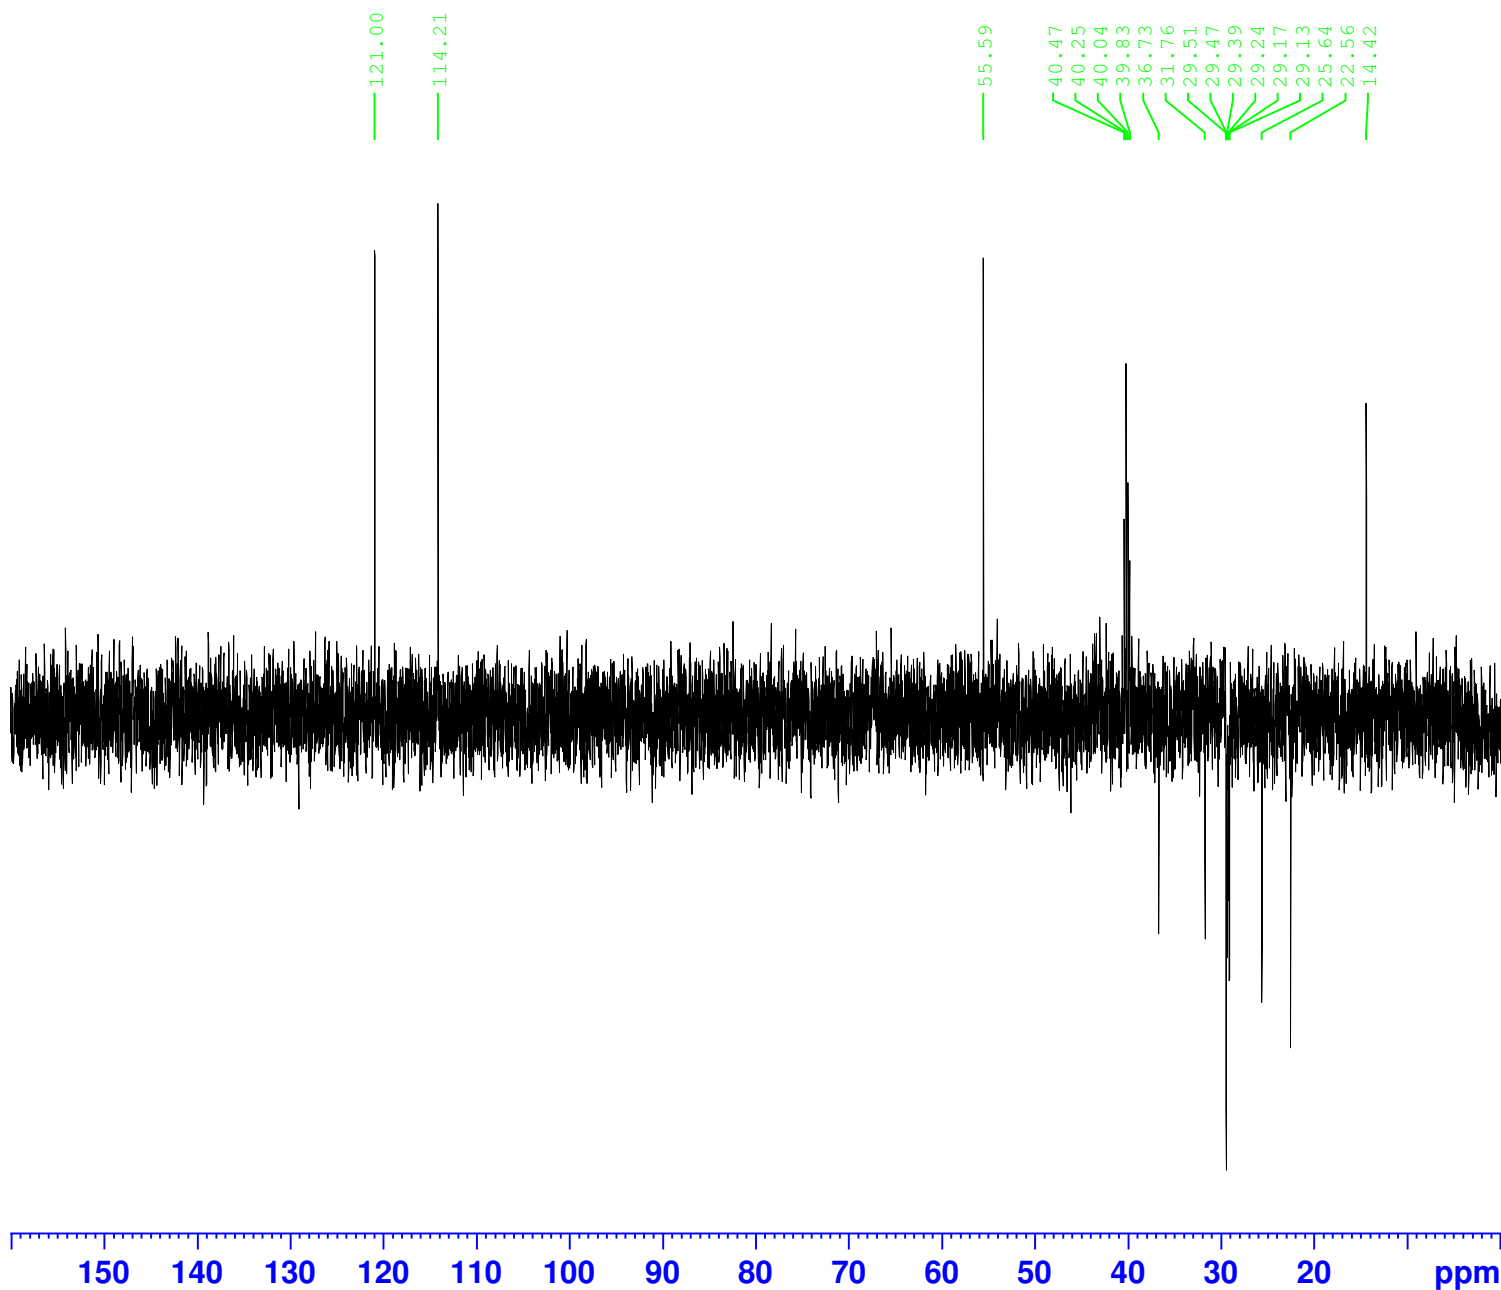

Current Data Parameters
 NAME nv2814fp1
 EXPNO 12
 PROCNO 1

F2 - Acquisition Parameters
 Date_ 20141129
 Time 2.40
 INSTRUM spect
 PROBHD 5 mm PABBO BB/
 PULPROG deptsp135
 TD 65536
 SOLVENT DMSO
 NS 256
 DS 4
 SWH 16129.032 Hz
 FIDRES 0.246110 Hz
 AQ 2.0316160 sec
 RG 212.69
 DW 31.000 usec
 DE 6.50 usec
 TE 298.0 K
 CNST2 145.0000000
 D1 2.0000000 sec
 D2 0.00344828 sec
 D12 0.00002000 sec
 TD0 1

===== CHANNEL f1 =====
 SFO1 100.6208171 MHz
 NUC1 13C
 P1 7.97 usec
 P13 2000.00 usec
 PLW0 0 W
 PLW1 101.00000000 W
 SPNAM[5] Crp60comp.4
 SPOAL5 0.500
 SPOFFS5 0 Hz
 SPW5 9.80230045 W

===== CHANNEL f2 =====
 SFO2 400.1312797 MHz
 NUC2 1H
 CPDPRG[2] waltz16
 P3 7.00 usec
 P4 14.00 usec
 PCPD2 70.00 usec
 PLW2 32.00000000 W
 PLW12 0.31999999 W

F2 - Processing parameters
 SI 32768
 SF 100.6127690 MHz
 WDW EM
 SSB 0
 LB 1.00 Hz
 GB 0
 PC 1.40