


AVIIHD400 [3]

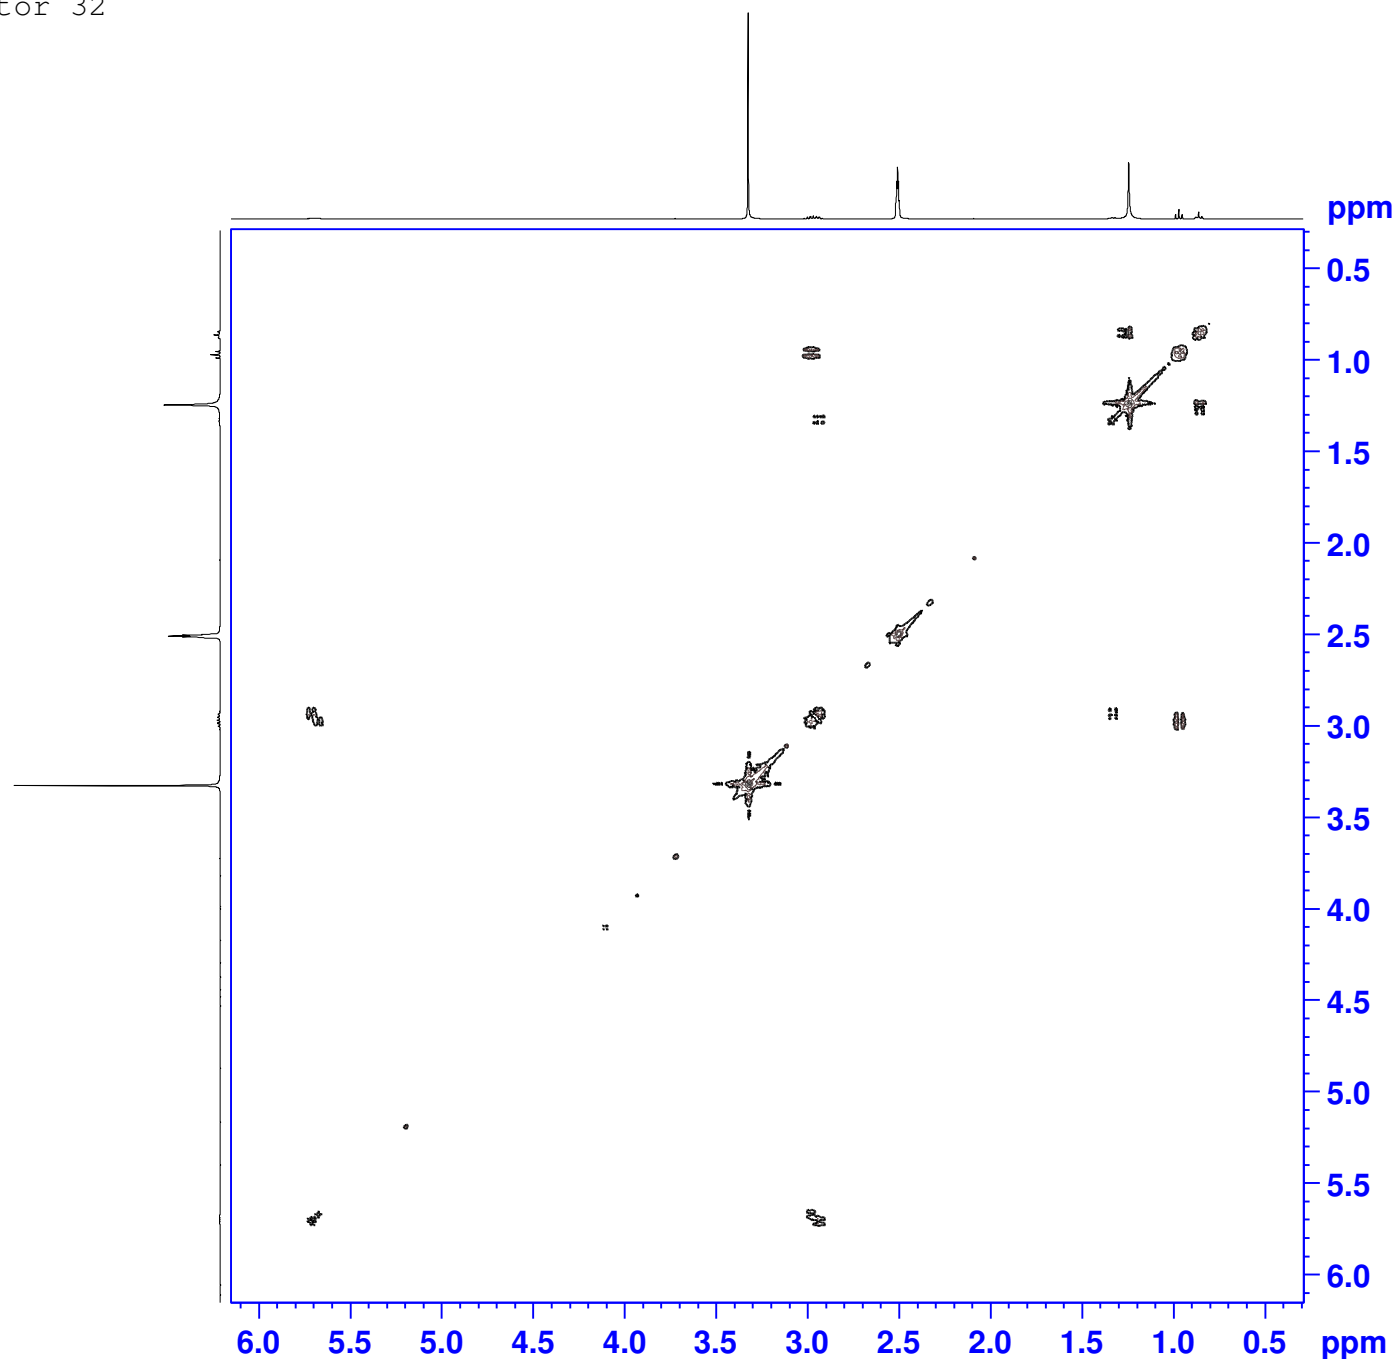

Current Data Parameters
NAME nv2814fp2
EXPNO 13
PROCNO 1

F2 - Acquisition Parameters
Date_ 20141129
Time 5.02
INSTRUM spect
PROBHD 5 mm PABBO BB/
PULPROG cosygpgqf
TD 2048
SOLVENT DMSO
NS 2
DS 8
SWH 2347.418 Hz
FIDRES 1.146200 Hz
AQ 0.4362240 sec
RG 58.58
DW 213.000 usec
DE 6.50 usec
TE 298.0 K
D0 0.00000300 sec
D1 1.31977403 sec
D13 0.00000400 sec
D16 0.00020000 sec
IN0 0.00042600 sec

===== CHANNEL f1 =====
SFO1 400.1312887 MHz
NUC1 1H
P0 7.00 usec
P1 7.00 usec
PLW1 32.00000000 W

===== GRADIENT CHANNEL =====
GPNAM[1] SMSQ10.100
GPZ1 10.00 %
P16 1000.00 usec

F1 - Acquisition parameters
TD 256
SFO1 400.1313 MHz
FIDRES 9.169600 Hz
SW 5.867 ppm
FnMODE QF

F2 - Processing parameters
SI 1024
SF 400.1300000 MHz
WDW SINE
SSB 0
LB 0 Hz
GB 0
PC 1.40

F1 - Processing parameters
SI 1024
MC2 QF
SF 400.1300000 MHz
WDW SINE
SSB 0
LB 0 Hz
GB 0